


# Mechanical Design Sketch Rev.3

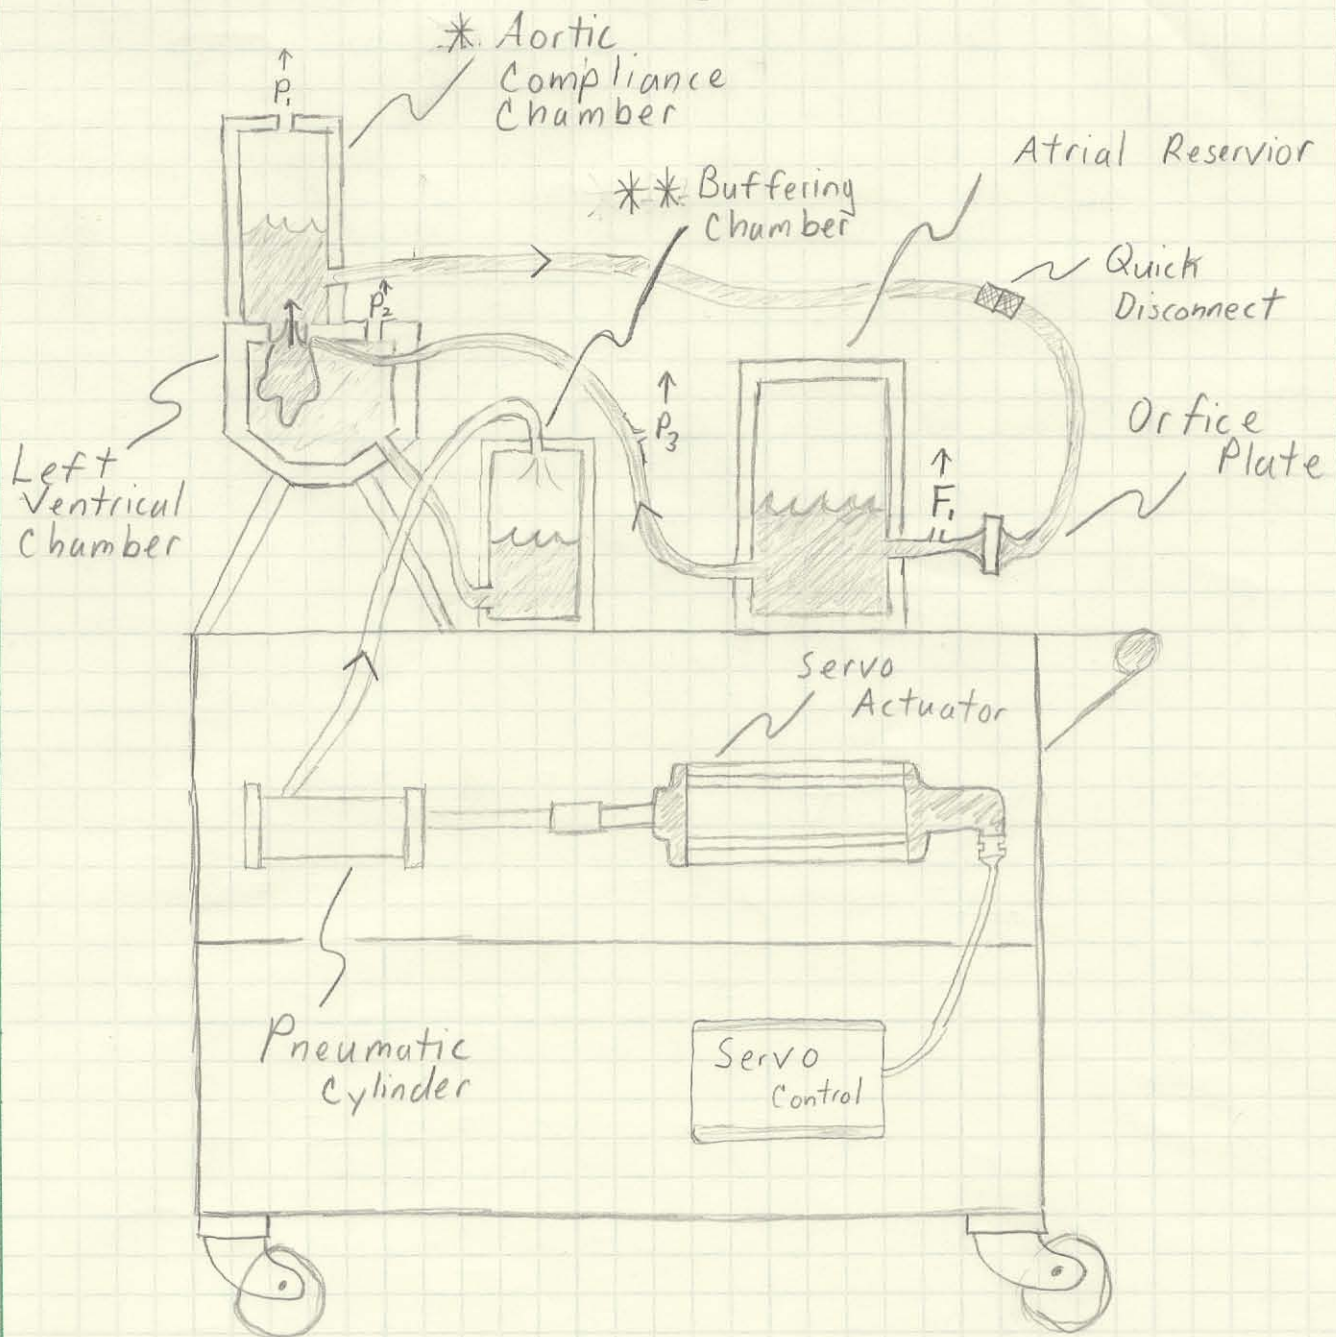

\* Aortic Compliance Chamber - moved closer to Ventricular Outlet to minimize losses

\*\* Buffering Chamber Added to prevent bubbles from interfering w/ ultrasound

P indicates Pressure tap to Control/Data system  
 F indicates Flow meter to Control/Data system